



**KENYA ACCREDITATION SERVICE**

P. O. Box 47400-00100, TEL. +254-787-395679, +254-725-227640 Nairobi, Kenya

Email: [info@kenyaaccreditation.org](mailto:info@kenyaaccreditation.org) Web: [www.kenas.go.ke](http://www.kenas.go.ke)

**SCHEDULE OF ACCREDITATION**

**NYERI WATER AND SANITATION COMPANY LIMITED**

**ISO/IEC 17025:2005**

Calibration Laboratory Number: **KENAS/CL/18**

Date of Accreditation: **23-Nov-2011**

Re-accreditation Decision: **16-Mar-2018**

**PERMANENT ADDRESS OF LABORATORY**

NYERI WATER AND SANITATION COMPANY - HEADQUARTERS

P. O. BOX 1520-10100

NYERI, KENYA

Tel: 2034548 / 2034623

Email: [info@nyewasco.co.ke](mailto:info@nyewasco.co.ke)

**Technical Manager:**

Mr. Peter G. Kahuthu

**Technical Signatories:**

1. Mr. Peter Kahuthu
2. Mr. Michael Mugo
3. Mr. Charles Waigera
4. Mr. Charles Wahome
5. Mr. James Gatuguta

Date of expiry: **22-Nov-2020**

Approved by:

  
KENAS CEO/Authorized Representative

Date: **24-Jun-2019**



## KENYA ACCREDITATION SERVICE

P. O. Box 47400-00100, TEL. +254-787-395679, +254-725-227640 Nairobi, Kenya

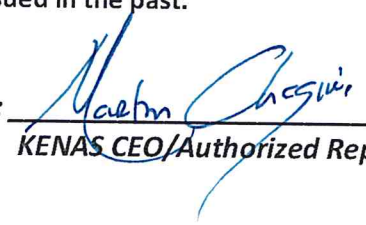
Email: [info@kenyaaccreditation.org](mailto:info@kenyaaccreditation.org) Web: [www.kenas.go.ke](http://www.kenas.go.ke)

### SCHEDULE OF ACCREDITATION

No	Calibration Field	Calibration Object	Measurand	Calibration Method	Standard	Calibration and Measurement Capability (CMC)  (Measurement Point /Range ± expanded uncertainty (k=2, level of confidence 95%))	Calibration Site
01	Flow Meter Calibration	Water Meters	Volumetric Flow rate	Internal Method: WSCO/02/TM/01 Reference Method: KS OIML R49:2004 (Part 1,2 & 3) Traceability: Cert. No. QASV/3L/NWSC/014/037	Calibration Bench Meter sizes 15mm to 40mm	0.015m <sup>3</sup> /hr to 20m <sup>3</sup> /hr ± 0.12%	Nyeri Water Central Lab and Clients Premises
				Internal Method: WSCO/02/TM/01 Reference Method: KS OIML R49:2004 (Part 1,2 & 3) Traceability: Cert. No. QASV/3L/NWSC/014/038			
				Internal Method: WSCO/02/TM/03 Reference Method: KS OIML R49:2004 (Part 1,2 & 3) Traceability Cert. No. BS/MET/8/3/47/098	Ultrasonic Flow Meter. Meter sizes 15mm to 1000mm	0.0m <sup>3</sup> /hr to 1000m <sup>3</sup> /hr ± 0.477m <sup>3</sup> /hr	
				Internal Method: WSCO/02/TM/03 Reference Method: KS OIML R49:2004 (Part 1,2 & 3) Traceability Cert. No. KEBS/BS/MET/8/3/47/099			
				Internal Method: WSCO/02/TM/03 Reference Method: KS OIML R49:2004 (Part 1,2 & 3) Traceability Cert. No. KEBS/BS/MET/8/3/47/100			

**Original Date of Accreditation: 23-Nov-2011**

This schedule is issued subject to the terms and conditions of KENAS Accreditation. It supersedes other schedule(s) issued in the past.

Approved by:  Date: 24-Jun-2019  
**KENAS CEO/Authorized Representative**